

Create a new era of rapid molecular diagnosis

# **iPonatic**

### Distribuido por:



Tel. +34 854 53 63 74 satcliente@Irdiagnostico.com www.Irdiagnostico.com



### **Product features**

#### Fast

Get result within 50 minutes

### Simple

Pre-packaged test strip
Room temperature preservation
Opening while using

### Easy


Easy to use
Integration of Extraction and
Amplification

#### Intelligence


Intelligent voice prompt


Analyse results automaticily

### **Test Results**

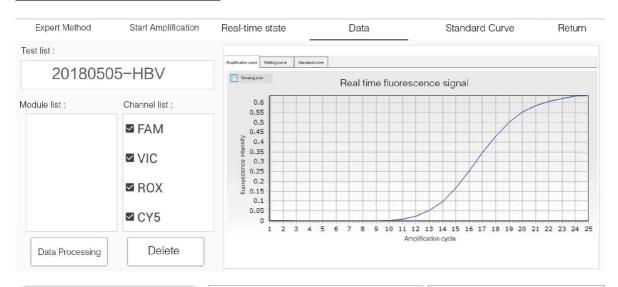

Data analysis of hundreds of samples shows that linear correlation R2 between iPonatic and manual operation reached 0.9667. At the same time, the systematic bias of the two groups of data is only ±0.01 log10. It means there is good consistency between iPonatic and manual operation.





### **Applicable Scenarios**

Community Healthcare

**Custom Quarantine** 

Medical Center



**Ambulance** 

Accident Scene

Others:such as Family Healthcare,
Infirmary,Drug Addiction Treatment Center
Public Security Department,Athlete Urine Test,etc.





# **iPonatic**

Portable Molecular Workstation

### Rapid

From sample to result within 30 minutes

### Easy

Intergration of extraction and amplification

## Simple

Pre-packed test strip Room temperature preservation Open while using

### Intelligent

Intelligent voice prompt Analyse result automatically

### Available Solutions

Novel Coronavirus Nucleic Acid Diagnostic Kit

4

Respiratory

Respiratory Pathogens Multiplex MP, ADV, BP

Hepatitis
HBV

5

Animal Detection

ASFV, PCV, MHP, PRV, FPV, FHV, FCrV

Maternal and Child Health
HPV 13+2, HPV6/11, HPV16/18
CT/UU/NG, CT/NG/MG, EB



Personalized medication
ALDH2&ADH1B, HLA-B27
MATHFR, CYP2C19



### **SAMPLING HANDLING AND PROCEDURE**




Fig1. Reagent carrier( within iPonatic)



Fig3. 25 ul PCR tube



Fig2. 4-Tube Strip



Fig4. 50 ul Filter tips

### Parameters

Ramp Rate Max 8°C (50-100°C)

Cooling Rate Max 2°C (50-100°C)

### Heatinging Technology:

Liquid metal coated ceramic heating/Air bath cooling

#### Temperature Control:

Independent heating module/ Independent module control

Temperature Accuracy ±0.3℃ (50℃~100℃)

Temperature Range ±5℃~99℃

Sample Volume 25ul/50ul

### Optical Unit

Light Source LED (maintenance-free)

Detector High sensitivity photoelectric sensor

Detection Mode Real-time dynamic monitoring

Channels 4

Excitation

Channel 1 Channel 2 Channel 3 Channel 4

470nm 525nm 580nm 635nm

Dyes FAM VIC ROX CY5

Seisitivity 1 copy

LOD <2nM (FAM/VIC/ROX/CY5)

### **FULL LIST OF CE-IVD CERTIFIED PARAMETERS**

Product	Product	Sample	Considiuitu	Result
section	name	type	Sensitivity	time
Hepatitis	HBV	Serum / plasma	300IU/ml	≤15min
series	HCV	Serum / plasma	-	≤40min
Maternal and child health series	HPV high-risk	Cervical exfoliated cell	1000 copies/ml	≤28min
	HPV13+2	Cervical exfoliated cell	1000 copies/ml	≤25min
	HPV6,11	Cervical exfoliated cell	800 copies/ml	≤25min
	HPV16,18	Cervical exfoliated cell	400 copies/ml	≤18min
	CT/UU/NG	Genital secretion	800 copies/ml	≤20min
	CT/NG/MG	Genital secretion	-	≤25min
	CT	Genital secretion	800 copies/ml	
	UU	Genital secretion	800 copies/ml	
	NG	Genital secretion	800 copies/ml	
	EB	plasma	1000 copies/ml	≤25min
Respiratory tract series	MP	Throat swab / sputum	400 copies/ml	≤18min
	respiratory tract upper 6	Throat swab	There was no significant difference between the detection limit of different pathogens and the original system	≤40min
	respiratory tract down 7	sputum	The detection limit of different pathogens for the original system is 2-4 times LOD	≤40min
	ADV	Pharyngeal swab	800 copies/ml	≤22min
	ВР	Pharyngeal swab	800 copies/ml	≤25min
Individualized medication series	ALDH2&ADH1B	Oral swab	-	≤18min
	HLA-B27	Oral swab	-	≤25min
	MATHFR	Oral swab	-	≤20min
	CYP2C19	Oral swab	-	≤20min
Public health	2019-nCoV	Nasopharynx swab	200 copies/ml	≤45min

### Distribuido por:

